

Study for Self-Treatment of Dementia by Biofeedback Rehabilitation

Ichiro Fukumoto^(✉)

Institute of Biomedical Engineering, Nagaoka University of Technology,
Kamitomioka 1603-1, Nagaoka, Japan
ichiro@vos.nagaokaut.ac.jp

Abstract. Light reflex and oculo-rotation analysing system is proposed in order to diagnose the Alzheimer type dementia (DAT) objectively. 19 patients are studied, which shows that the maximum miosis ratio and miosis velocity are sensitive parameters to evaluate the severity of dementia and the changing time of internal and external rectus eye muscles is the effective index for screening of the dementia. The threshold of the changing time over 0.35 s can discriminate DAT clearly from the normal. Biofeedback trainings of the demented are executed by the objective diagnosing method, which shows improvement in MMSE, ADL score and the eye reflex parameters. The proposed method may become a safe non-pharmacological treatment of the dementia.

Keywords: Alzheimer type dementia · Physiological diagnosis · Light reflex · Eye pursuit · Biofeedback rehabilitation

1 Introduction

The number of Alzheimer dementia patients (AD) is supposed to become almost 5 million in Japan by 2030. As the aetiology is unknown, the early diagnosis is important in order to slow down the aggravation by donepezil and brain rehabilitations. The screening methods are not only subjective (MMSE, HDS-R etc.) but also time consuming (15–45 min) in the early stage, when the brain imaging (CT, MRI or PET) is neither so effective nor decisive in this period.

We have found the abnormality of eye reflexes in Alzheimer dementia patients, that is rapid and objective and it can be widely used from the early to the final stage of dementia evaluation even in ordinary primary care settings.

As we believe that every medical diagnosis should contribute patients' cure and care, we have studied the effect of non-pharmacological treatment of the dementia by peripheral stimulations including electrical current or visible light with the new diagnosing systems. About 40 % of the AD patients have revealed the improved MMSE scores in short period after the treatment.

In this study we also try to apply the biofeedback training for self-cure by AD patients' themselves adding to the former electrical stimulations on acute points. The result is rather encouraging with the effect of 50 %, so we hope that our proposed complex treating method might become a safe and self-cure even in the AD patients' homes.

2 New Objective Diagnosing Methods

Scinto et al. found that the pupil midriatic time response by tropicamide in AD patients were abnormal (Scinto: Science, 266 p. 1051.1994) [1–14, 19, 20]. But his method is not only unavailable especially for elders with glaucoma and also unstable and time consuming (about 1 h). We have improved the shortcomings by using visible light stimulation instead of midriatic medicine and by measuring constricting speed (Fig. 1) [15–18].

The original system has the following features.

- Light stimulation by small lamp
- Infrared CCD camera detected pupil image
- Automatically calculated diameter of the pupil by a personal computer.

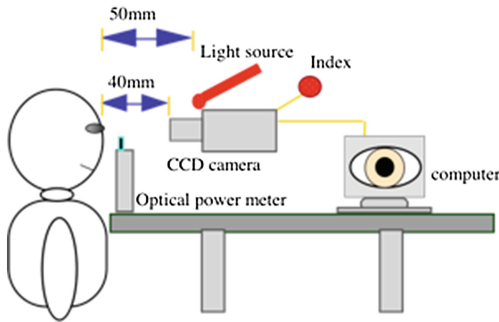


Fig. 1. Light reflex measuring system

We have found that the pupil constriction (= miosis) of the demented patient by visible light stimulation is less in the response size and slower than the normal elders (Fig. 2) [21–23].

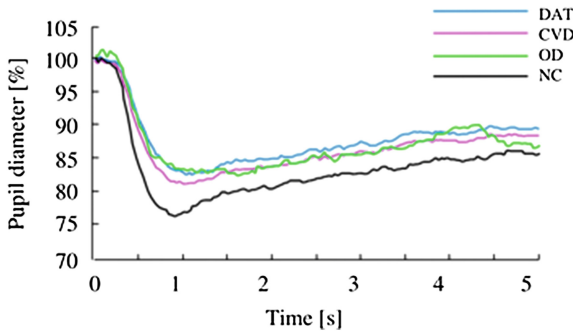


Fig. 2. Light reflex curves of the dementia (DAT: Alzheimer dementia, CVD: Cerebro-vascular dementia, OD: Dementia of other type, NC: Normal control)

Several parameters are calculated from the light reflex curve (Fig. 3). Maximum miosis ratio and 10 %-90 % Miosis velocity are most sensitive parameters to evaluate the severity of dementia.

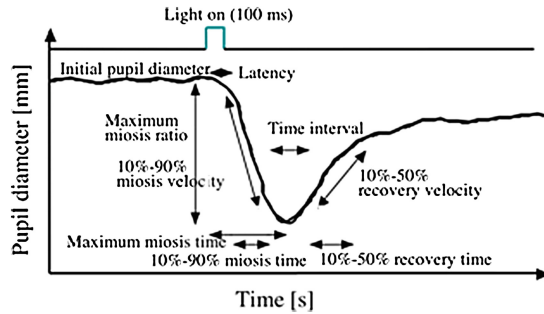


Fig. 3. Light reflex parameters

The 83 clinically diagnosed demented patients and 32 normal elders are tested as the subjects for the system. All type of the dementia can be discriminated by the miotic time (Mt) with $p < 0.05$ or 0.01 (Fig. 4).

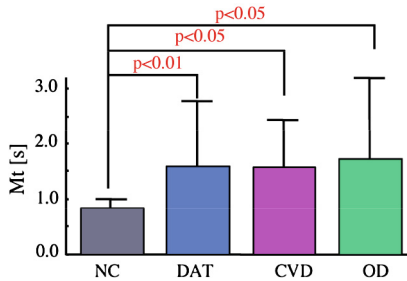


Fig. 4. The miotic time (Mt)

The two-group discriminant analysis of the light reflex (Table 1) shows sensitivity (88 %), specificity (97 %), positive correction probability (90 %), and LR + (Likelihood ratio for a positive finding: 28).

Table 1. Two-group discriminant analysis

		Clinical Diagnosis	
		Dementia	Control
Light Reflex	Subjects		
	Dementia	73	1
	Normal	10	31

To improve the original system we add an eye tracking mechanism and construct an improved eye reflex and tracking-diagnosing units (Fig. 5) [24–27].



Fig. 5. The improved measuring unit with gaugle

The subjects are 19 demented patients; AD (75.1 ± 5.9 years old, HDS-R = 11.3 ± 7.7), 18 normal elders; EC (79.5 ± 7.4 years old, HDS-R = 27.9 ± 3.4) and 7 healthy young volunteers; YC (24.9 ± 4.8 years old, HDS-R = 30.0). Subjects are instructed to wear a glass-type attachment that includes a small LCD monitor and a CCD digital camera. They are also instructed to track a small black dot running on a horizontal line in the LCD monitor from the right to left and vice versa randomly. The velocities of pursuing target are 300, 400 and 500 pixel/s. The location of an eye’s pupil center is automatically calculated using cornea light reflex method by a built-in processing unit in the system through the CCD camera.

The oculogyration responses are calculated from the pupil center location data afterward and are visualized as simple time versus eye-location curves in an off line batch process of connected another desktop type personal computer. As diagnosing parameters, we have adopted the switching time of internal and external rectus muscles, velocities, peak values, the averaged difference between the patient and the normal.

AD patients show the weaker and slower tracking curves than the normal elders (Fig. 6). Especially the changing time of m. rectus lateralis and medialis seems to be the most sensitive parameter.

Especially the changing time between the outer and inner muscles has clear negative correlation ($r = -0.72$) with MMSE and all AD patients have the changing time of over 0.35 s (Fig. 7).

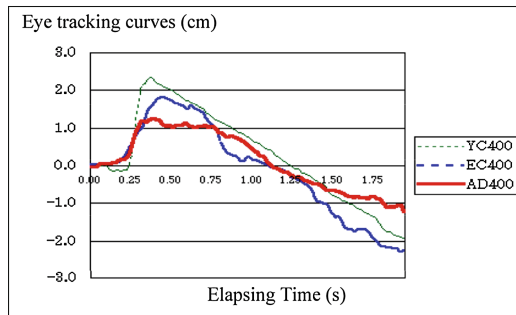


Fig. 6. An eye tracking curves (AD: Alzheimer, EC: normal elder, YC: normal young)

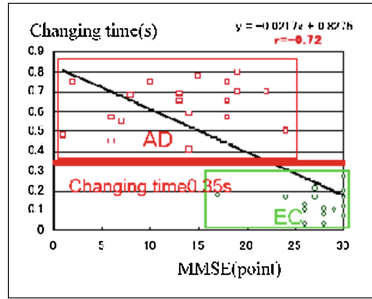


Fig. 7. The changing time of the outer and inner rectus muscles.

The two objective diagnosing methods with light reflex and eye tracking seem to be useful and effective enough not only for the screening but also for the biofeedback rehabilitation of the dementia.

3 Rehabilitation of the Dementia

As the aetiology and aggravation mechanism of dementia are both unknown, no fundamental treatment is developed by now. Only donepezil is used to retard the progression but the effect is restricted in about 0.5 to 2 years.

On the other hand it is said that only 10 % of the 14 billions human neurons are used in his/her life and that neurons can be newly yielded in need. If the damaged neurons in the dementia are possible to re-activated or re-produced by outer stimulation, we believe that non-medical treatment should be realized.

We are studying the dementia improving effect with stimulating energy (mechanical, electrical and visual) on patients' peripheral nerves and the biofeedback rehabilitation technique.

The biofeedback (BF) is the process of gaining greater awareness of many physiological functions primarily using instruments that provide information on the activity of those same systems, with a goal of being able to manipulate them at will. BF may be used to improve health, performance, and the physiological changes which often occur in conjunction with changes to thoughts, emotions, and behavior. The BF has been found to be effective for the treatment of headaches and migraines. It can be said to be one kind of body-mind interactive self-treatment that has same aim of integrated medicine (Fig. 8).

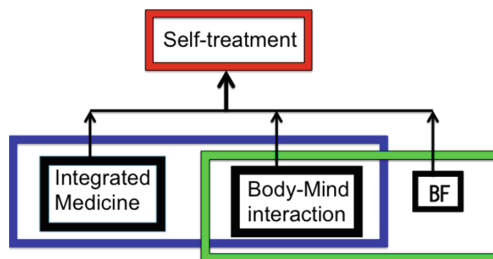


Fig. 8. Biofeedback and Body-mind interaction

If we could get good biological information and stimulation, BF may become a new rehabilitation method for the dementia patient (Fig. 9). In this study we mainly apply the eye reflex as the feedback parameter (= output) and several energy for the peripheral stimulation (= input) (Fig. 9).

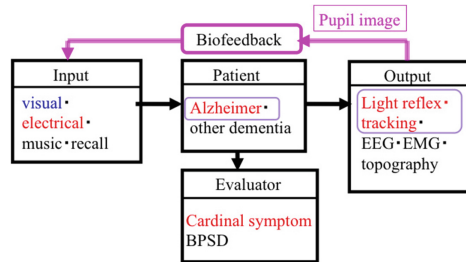


Fig. 9. Biofeedback system for the dementia

3.1 Mechanical Stimulation

In oriental medicine mechanical stimulation such as acupuncture (= Sinkyu) or finger pressure (= Shiatsu) is widely used for non-pharmacological treatment of diverse diseases. Especially they are effective for nervous system disorder (e.g.: neuralgia, paralysis, convulsions, stroke recovery, polio, insomnia), we assume it may be applicable to the dementia.

A commercial foot-sole patting machine is used for the mechanical stimulation on acute point KI01 (Yuusen) in 13 dementia patients (81.7 ± 3.8 years old). The treatment is executed for 15 min × 2 times a week during 1 month.

The averaged MMSE of the patient are improved from 20.8 to 23.0 (Fig. 10).

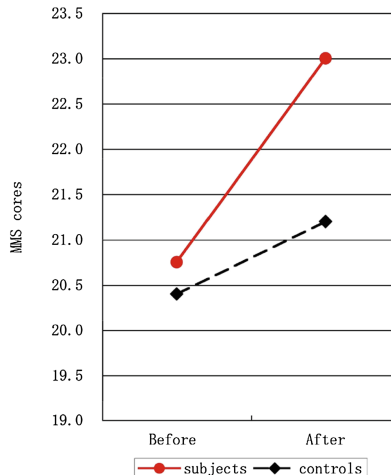


Fig. 10. Mechanical stimulation on foot sole

The ADL of the patients is also improved especially in affective aspect. Is also improved especially in affective aspect and abnormal behaviours ($p < 0.01$).

3.2 Electric Stimulation

TENS (transcutaneous electrical nerve stimulation) on acute points is also widely used as a variation of acupuncture. A commercial TENS apparatus (Trio300, 0.3–400 Hz, Burst wave 25 mA) is applied to 11 dementia patients (mild 5 + severe 6, 75.6 years old) for 30 min/day, 3 times/week for 1 month. Stimulating point is Seimei (BL1) that is an acute point for relief of headache and asthenopia (Fig. 11).

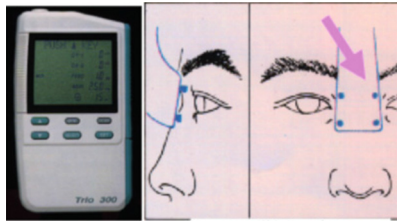


Fig. 11. TENS apparatus and acute point BL1

HDS-R is improved from 10.3 ± 5.0 to 14.3 ± 6.2 in mild group and from 3.7 ± 1.6 to 6.0 ± 5.4 in severe group. SMT-7 and the light reflex parameters are also improved in all patients [28–30].

3.3 Light Stimulation

Light stimulation by LED in the gaugle (1 s, 5 times/min., 3 trials a day for 3 days) is tried for 15 DAT patient 15 (81.6 years old, $\sigma 5 \text{ } \eta 10$) and CVT patients (75.6 years old, $\sigma 2 \text{ } \eta 3$). HDS-R scores of 3 AD and all 5 CVD patients are improved. The light reflex parameters are also improved (Fig. 12).

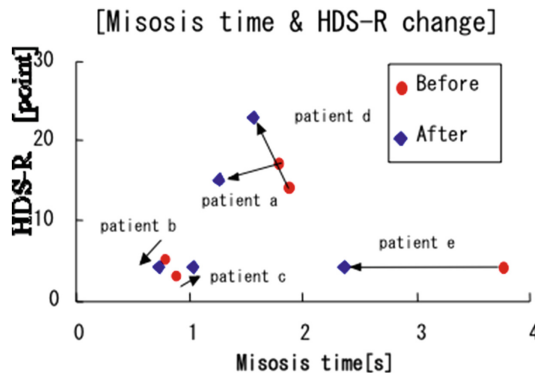


Fig. 12. HDS-R change and Light reflex parameter change by light stimulation.

3.4 Comparison of Peripheral Stimulation Effect

Comparing the three stimulating energy on the peripheral sensor, the light and the electric stimulation are more effective for dementia improvement than the mechanical one (Fig. 13).

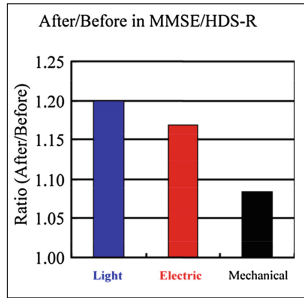


Fig. 13. Comparison of three types of stimulation

3.5 Biofeedback Rehabilitation

Expecting the better improving effect, we propose a new complex treatment by TENS and visual biofeedback.

TENS on acute point BL-1 is used as peripheral nerve stimulation. At the same time the visual images of pupils are presented to the patients as biofeedback signals (Fig. 14).

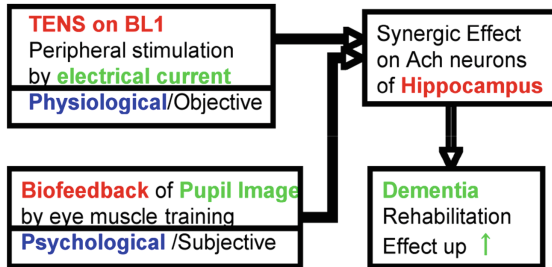


Fig. 14. Complex treatment by TENS and visual biofeedback

Subjects are Alzheimer dementia patients 4 (♂1, ♀3, 77.0 ± 7.4 years old, HDS-R: 16.0 ± 4.4; MMSE: 17.3 ± 6.0).

Treatment is total 10 trials, each 30 min., every other day. The peripheral stimulation is given by TENS of the acute point “Seimei-ketsu”(BL1). The biofeedback signal is the visual images of patients’ pupils. MMSE, HDS-R and 7 memorizing items are tested as the intellectual evaluators. The latency time, light reflex time, speed and the inner-outer straight muscle changing time is measured as the physiological evaluators. N-ADL scale and N-M scale are also done as the ADL evaluator.

The results of the complex treatment show higher effect for improvement of the dementia in MMSE/HDS-R as well as the physiological parameters than the simple peripheral stimulations (Figs. 15 and 16).

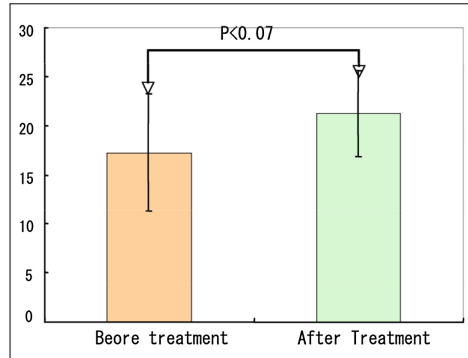


Fig. 15. MMSE improvement by complex treatment of TENS and the visual biofeedback

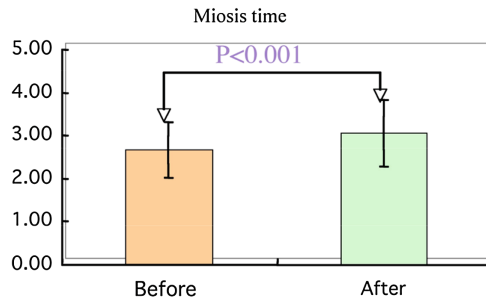


Fig. 16. Miotic time improvement by complex treatment

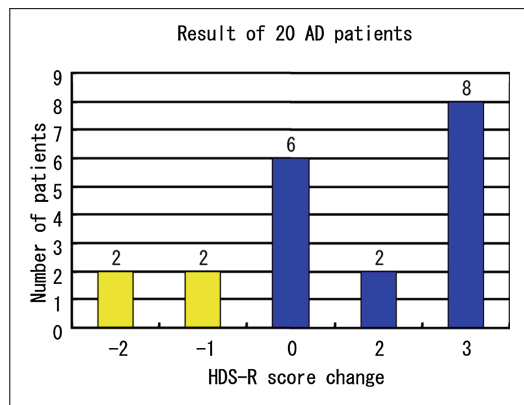


Fig. 17. Result of the extended trial

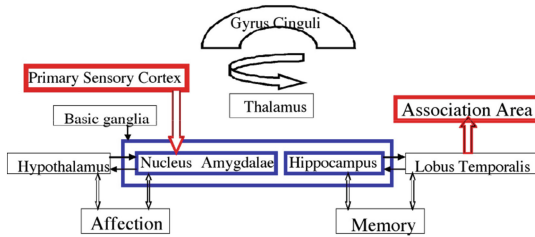


Fig. 18. A neural model of CNS modulation by peripheral stimulation

The extended trial shows that the 10 out of the 20 Alzheimer patients are improved in HDS-R by the complex treatment. The complex treatment with biofeedback is more effective (50 %) than the TENS only treatment (40 %) even in the scaled up trial (Fig. 17).

The peripheral sensory stimulation may modulate the signals from Hypothalamus to Lobus temporalis in Nucleus amygdalae/Hippocampus (Fig. 18). The method might yield a new non-pharmacological arsenal for the treatment of dementia [23].

4 Conclusions

The light reflex and eye tracking parameters are adopted as the physiological evaluators for Alzheimer dementia.

TENS on acute point BL-1 is used as peripheral nerve stimulation. At the same time the visual images of pupils are presented to the patients as biofeedback signals.

The results of the complex treatment show higher effect for improvement of the dementia in MMSE/HDS-R as well as the physiological parameters than the simple peripheral stimulations.

The method might yield new non-pharmacological arsenals for the treatment of dementia.

Acknowledgements. We would like to extend sincere thanks to the patients and the staffs of Mishima hospital. We owe Dr.Fukushima in Panasonic Denko, who kindly helps development of the diagnosing system of the dementia. As the experiments are executed by the earnest foreign doctor students (Shi Xuemin and Guo Yi) as well as Dr Hisashi UCHIYAMA in our institute, we should say hearty thanks to them.

References

1. Sekuler, R., Hutman, L.P., Owsley, C.J.: Human aging and spatial vision. *Science* **209**, 1255–1256 (1980)
2. Jones, A., Friedland, R.P., Koss, B., Stark, L., Thompkins-Ober, B.A.: Saccadic intrusions in Alzheimer-type dementia. *J. Neurol.* **229**, 189–194 (1983)

3. Hutton, J.T., Nagel, J.A., Loewenson, R.B.: Eye tracking dysfunction in Alzheimer-type dementia. *Neurology* **34**, 99–102 (1984)
4. Lisberger, S.G., Morris, E.J., Tychsen, L.: Visual motion processing and sensory-motor integration for smooth pursuit eye movements. *Annu. Rev. Neuro-sci.* **10**, 97–129 (1987)
5. Robinson, D.A., Gordon, J.L., Gordon, S.E.: A model of the smooth pursuit eye movement system. *Biol. Cybern.* **55**, 43–57 (1988)
6. Fletcher, W.A., Sharpe, J.A.: Smooth pursuit dysfunction in Alzheimer's disease. *Neurology* **38**, 272–277 (1988)
7. Mendez, M.F., Tomsak, R.L., Remler, B.: Disorders of the visual system in Alzheimer's disease. *J. Clin. Neuro-ophthalmol.* **10**(1), 62–69 (1990)
8. Trick, G.L., Silverman, S.E.: Visual sensitivity to motion: age-related changes and deficits in senile dementia of the Alzheimer type. *Neurology* **41**, 1437–1440 (1991)
9. Cronin-Golomb, A., Corkin, S., Rizzo, J.F., Cohen, J., Growdon, J.H., Banks, K.S.: Visual dysfunction in Alzheimer's disease: relation to normal age. *Ann. Neurol.* **29**(1), 41–52 (1991)
10. Müller, G., Richter, R.A., Weisbrod, S., Klingberg, F.: Impaired eye tracking performance in patients with presenile onset dementia. *Int. J. Psychophysiolol.* **11**, 167–177 (1991)
11. Zaccara, G., Gangemi, P.F., Muscas, G.C., Paganini, M., Pallanti, S., Parigi, A., Messori, A., Arnetoli, G.: Smooth-pursuit eye movements: alterations in Alzheimer's disease. *J. Neurol. Sci.* **112**, 81–89 (1992)
12. Scinto, L.F.M., Daffner, K.R., Castro, L., Weintraub, S., Vavrik, M., Mesulam, M.M.: Impairment of spatially directed attention in patients with probable Alzheimer's disease as measured by eye movements. *Arch. Neurol.* **1**, 682–688 (1994)
13. Paasuraman, R., Greenwood, P.M., Alexander, G.E.: Selective impairment of spatial attention during visual search in Alzheimer's disease. *Cogn. Neurosci. Neuropsychol., Neuro Report* **6** 6(14), 1861–1864 (1995)
14. Moser, A., Kömpf, D., Olschinka, J.: Eye movement dysfunction in Dementia of the Alzheimer type. *Dementia* **6**, 264–268 (1995)
15. Shi, X., Utiyama, H., Fukumoto, I.: A study for diagnose dementia using miosis by light-reflex. In: *International Symposium on Dementia – from Molecular Biology to Therapeutics*, Kobe, p. 46, 11–13 September 1999
16. Fukumoto, I.: A computer simulation of the new diagnosing method by human eye light-reflexes. In: *Proceedings of IEEE-EMBS Asia-Pacific Conference on Biomedical Engineering (APBME2000)*, pp. 624–625, 26 September 2000
17. Shi, X., Guo, Y., Uchiyama, H., Fukumoto, I.: A Study for a new Diagnostic and Rehabilitation method for Dementia Using miosis by Light-Reflex. In: *Proceedings of IEEE-EMBS Asia-Pacific Conference on Biomedical Engineering (APBME2000)*, pp. 505–506, 28 September 2000
18. Fukushima, S., Shi, X., Tsuchida, Y., Guo, Y., Uchiyama, H., Fukumoto, I., Suzuki, K., Murakami, S., Nakajima, R.: A new objective approach to diagnose dementia by pupillary light reflex method. In: *Proceedings of IEEE-EMBS Asia-Pacific Conference on Biomedical Engineering (APBME2000)*, pp. 716–717, 28 September 2000
19. Rösler, A., Mapstone, M.E., Hays, A.K., Mesulam, M.M., Rademaker, A.: Alterations of visual search strategy in Alzheimer's Disease and Aging. *Neuropsychology* **14**(3), 398–408 (2000)
20. Lueck, K.L., Mendez, M.F., Perryman, K.M.: Eye movement abnormalities during reading in patients with Alzheimer disease. *Neuropsychiatry, Neuropsychol. Behav. Neurol.* **13**(2), 77–82 (2000)

21. Fukumoto, I.: A computer simulation of the new diagnosing method by human eye light-reflexes. In: Proceedings of IEEE-EMBS Asia-Pacific Conference on Biomedical Engineering (APBME2000), Hanzhou, pp. 624–625, 26 September 2000
22. Fukumoto, I.: A basic study for the new dementia diagnostic system using human eye light reflex. In: Proceeding of the International Workshop on Gerontechnology, Tsukuba, pp. 93–94, 13 March 2001
23. Fukumoto, Ichiro: Computer aided diagnosis for the Alzheimer type dementia. In: Niessen, Wiro J., Viergever, Max A. (eds.) MICCAI 2001. LNCS, vol. 2208, pp. 1386–1387. Springer, Heidelberg (2001)
24. Fukumoto, I.: A computer diagnosing system of dementia using smooth pursuit oculogyration. In: Dohi, T., Kikinis, R. (eds.) MICCAI 2002, Part I. LNCS, vol. 2488, pp. 674–681. Springer, Heidelberg (2002)
25. Fukumoto, I.: New diagnosing system for the automatic screening of Alzheimer type dementia by human eye reflexes. In: Proceedings of International Congress on Biological and Medical Engineering, D1VB-1230, Singapore, December 2002
26. Guo, Y., Shi, X., Uchiyama, H., Hasegawa, A., Nakagawa, Y., Tanaka, M., Fukumoto, I.: A study of the rehabilitation of cognitive function and short-term memory in patients with Alzheimer's disease using transcutaneous electrical nerve stimulation. *Frontiers Med. Biol. Eng.* **11**(4), 237–247 (2002)
27. Fukumoto, I.: A study of physiological diagnosing system for Alzheimer type dementia by oculomotor dysfunction. In: The Congress Proceedings of World Congress on Medical Physics and Biomedical Engineering, Sydney, 24–29 August 2003
28. Fukumoto, I., Guo, Y., Hasegawa, J., Shi, X.: Rehabilitation systems of Alzheimer type dementia by somatic stimulations. *Transactions of the Japanese Society for Medical and Biological Engineering*, 665 (2005) (Tsukuba)
29. Fukumoto, I.: A unified model of the Alzheimer-dementia and Parkinsonian-disease based on the somatic stimulation effects. In: WC 2006 Program Book, Seoul, pp. 125–128, August 2006
30. Fukumoto, I.: A Study for physiological diagnosis and non-pharmacological treatment of the Alzheimer type dementia. In: *Healthinf 2011* (2011)
31. Fukumoto, I.: Physiological diagnosis and rehabilitation for the Alzheimer type dementia. In: Imamura, K., Usui, S., Shirao, T., Kasamatsu, T., Schwabe, L., Zhong, N. (eds.) *BHI 2013*. LNCS, vol. 8211, pp. 324–335. Springer, Heidelberg (2013)